

HI97101

pH, Free Chlorine,
Total Chlorine, Cyanuric Acid,
Iron Low Range,
Bromine & Iodine
Photometer



INSTRUCTION MANUAL

**Dear
Customer,**

Thank you for choosing a Hanna Instruments product.

Please read this instruction manual carefully before using this instrument.

This manual will provide you with the necessary information for correct use of this instrument, as well as a precise idea of its versatility.

If you need additional technical information, do not hesitate to e-mail us at tech@hannainst.com or view our worldwide contact list at www.hannainst.com.

All rights are reserved. Reproduction in whole or in part is prohibited without the written consent of the copyright owner, Hanna Instruments Inc., Woonsocket, Rhode Island, 02895, USA.

TABLE OF CONTENTS

1. PRELIMINARY EXAMINATION	5
2. SAFETY MEASURES.....	6
3. ABBREVIATIONS	6
4. SPECIFICATIONS.....	7
5. DESCRIPTION	9
5.1. GENERAL DESCRIPTION & INTENDED USE.....	9
5.2. FUNCTIONAL DESCRIPTION	10
5.3. PRECISION & ACCURACY.....	11
5.4. PRINCIPLE OF OPERATION	11
5.5. OPTICAL SYSTEM.....	12
6. GENERAL OPERATIONS.....	13
6.1. METER VALIDATION: CAL CHECK & CALIBRATION.....	13
6.2. GLP.....	15
6.3. LOGGING DATA & LOG RECALL	16
6.4. GENERAL SETUP	17
6.5. REAGENTS & ACCESSORIES.....	19
6.6. CONTEXTUAL HELP.....	19
6.7. BATTERY MANAGEMENT	20
7. PHOTOMETER.....	21
7.1. METHOD SELECTION	21
7.2. COLLECTING & MEASURING REAGENTS AND SAMPLES.....	21
7.3. CUVETTE PREPARATION	22
8. METHOD PROCEDURE	24
8.1. pH.....	24
8.2. FREE CHLORINE (POWDER REAGENT)	26
8.3. FREE CHLORINE (LIQUID REAGENT)	28
8.4. TOTAL CHLORINE (POWDER REAGENT).....	31
8.5. TOTAL CHLORINE (LIQUID REAGENT)	33
8.6. CYANURIC ACID.....	36
8.7. IRON LOW RANGE.....	38
8.8. BROMINE.....	41
8.9. IODINE	43

9. WARNING & ERROR DESCRIPTIONS.....	45
10. BATTERY REPLACEMENT	47
11. ACCESSORIES.....	48
11.1. REAGENT SETS.....	48
11.2. OTHER ACCESSORIES	49
CERTIFICATION.....	50
RECOMMENDATIONS FOR USERS.....	50
WARRANTY	50

1. PRELIMINARY EXAMINATION

Remove the instrument and accessories from the packaging and examine it carefully. For further assistance, please contact your local Hanna Instruments Office or email us at tech@hannainst.com.

Each **HI97101C** is delivered in a rugged carrying case and is supplied with:

- Sample cuvette (2 pcs.)
- Sample cuvette cap (2 pcs.)
- Plastic stopper (2 pcs.)
- **A ZERO** - CAL Check Cuvette A
- **HI97701B** - CAL Check Cuvette B for Free and Total Chlorine (Powder & Liquid)
- **HI97710B** - CAL Check Cuvette B for pH
- **HI97716B** - CAL Check Cuvette B for Bromine
- **HI97718B** - CAL Check Cuvette B for Iodine
- **HI97722B** - CAL Check Cuvette B for Cyanuric Acid
- **HI97746B** - CAL Check Cuvette B for Iron Low Range
- Cloth for wiping cuvettes
- Scissors
- 1.5V AA Alkaline batteries
- CAL Check standard certificate
- Instrument quality certificate
- Instruction manual

Each **HI97101** is delivered in a cardboard box and is supplied with:

- Sample cuvette (2 pcs.)
- Sample cuvette cap (2 pcs.)
- Plastic stopper (2 pcs.)
- 1.5V AA Alkaline batteries
- Instrument quality certificate
- Instruction manual

Note: Save all packing material until you are sure that the instrument works correctly. Any damaged or defective item must be returned in its original packing material with the supplied accessories.

2. SAFETY MEASURES



- The chemicals contained in the reagent kits may be hazardous if improperly handled.
- Read the Safety Data Sheets (SDS) before performing tests.
- Safety equipment: Wear suitable eye protection and clothing when required, and follow instructions carefully.
- Reagent spills: If a reagent spill occurs, wipe up immediately and rinse with plenty of water. If reagent contacts skin, rinse the affected area thoroughly with water. Avoid breathing released vapors.
- Waste disposal: For proper disposal of reagent kits and reacted samples, contact a licensed waste disposal provider.

3. ABBREVIATIONS

mg/L	milligrams per liter (ppm)
mL	milliliter
°C	degree Celsius
°F	degree Fahrenheit
DIW	Deionized Water
EPA	US Environmental Protection Agency
DPD	N,N-diethyl-p-phenylenediamine
GLP	Good Laboratory Practice
HDPE	High Density Polyethylene
LED	Light Emitting Diode
LR	Low Range
NIST	National Institute of Standards and Technology

4. SPECIFICATIONS

pH	Range	6.5 to 8.5 pH
	Resolution	0.1 pH
	Accuracy	± 0.1 pH of reading at 25 °C
	Method	Adaptation of the Phenol Red Method
Chlorine (All Methods)	Range	0.00 to 5.00 mg/L (as Cl ₂)
	Resolution	0.01 mg/L
	Accuracy	± 0.03 mg/L $\pm 3\%$ of reading at 25 °C
Cyanuric Acid	Method	Adaptation of the US EPA Method 330.5, DPD Colorimetric Method
	Range	0 to 80 mg/L (as CYA)
	Resolution	1 mg/L
	Accuracy	± 1 mg/L $\pm 15\%$ of reading at 25 °C
Iron LR	Method	Adaptation of the Turbidimetric Method
	Range	0.00 to 1.60 mg/L (as Fe)
	Resolution	0.01 mg/L
Bromine	Accuracy	± 0.01 mg/L $\pm 8\%$ of reading at 25 °C
	Method	Adaptation of the TPTZ Method
	Range	0.00 to 10.00 mg/L (as Br ₂)
	Resolution	0.01 mg/L
Iodine	Accuracy	± 0.08 mg/L $\pm 3\%$ of reading at 25 °C
	Method	Adaptation of Standard Methods for the Examination of Water and Wastewater, 18 th Edition, DPD Method
	Range	0.0 to 12.5 mg/L (as I ₂)
	Resolution	0.1 mg/L
Iodine	Accuracy	± 0.1 mg/L $\pm 5\%$ of reading at 25 °C
	Method	Adaptation of Standard Methods for the Examination of Water and Wastewater, 18 th Edition, DPD Method

Measurement System	Light source	Light Emitting Diode
	Bandpass filter	525 nm
	Bandpass filter bandwidth	8 nm
	Bandpass filter wavelength accuracy	± 1.0 nm
	Light detector	Silicon photocell
	Cuvette type	Round 24.6 mm diameter (22 mm inside)
Additional Specifications	Auto logging	50 readings
	Display	128 x 64 pixel B/W LCD with backlight
	Auto-off	After 15 minutes of inactivity (30 minutes before a READ measurement)
	Battery type	1.5 V AA Alkaline (3 pcs.)
	Battery life	> 800 measurements (without backlight)
	Environment	0 to 50 °C (32 to 122 °F); 0 to 100% RH, non-serviceable
	Dimensions	142.5 x 102.5 x 50.5 mm (5.6 x 4.0 x 2.0")
	Weight (with batteries)	380 g (13.4 oz.)
	Case ingress protection rating	IP67, floating case

5. DESCRIPTION

5.1. GENERAL DESCRIPTION & INTENDED USE

The **HI97101** is an auto-diagnostic portable meter that benefits from Hanna's years of experience as a manufacturer of analytical instruments. It has an advanced optical system that uses a Light Emitting Diode (LED) and a narrow band interference filter that allows for accurate and repeatable readings.

The optical system is sealed from outside dust, dirt and water. The meter uses an exclusive positive-locking system to ensure that the cuvettes are placed into the holder in the same position every time.

With the CAL Check™ functionality, users are able to validate the performance of the instrument at any time and apply a user calibration (if necessary). Hanna Instruments CAL Check cuvettes are made with NIST traceable standards.

The built-in tutorial mode guides users step-by-step through the measurement process. It includes all steps required for sample preparation, the required reagents and quantities.

The **HI97101** meter measures seven important parameters in the treatment and disinfection of drinking water, wastewater and swimming pools.

Bromine and chlorine are widely used disinfectants. In order for chlorine to be effective the pH of the water should be less than 8.0. The method for pH is an adaptation of the Phenol Red Method, for chlorine is an adaptation of the US EPA Method 330.5, DPD Colorimetric Method and for bromine is an adaptation of Standard Methods for the Examination of Water and Wastewater, 18th Edition, DPD Method.

Cyanuric Acid is added to increase the life of chlorine, without it chlorine levels can be reduced by up to 90% in hours, when exposed to sunlight. The method for cyanuric acid is an adaptation of the Turbidimetric Method.


Iron is present in drinking water in low concentrations, the solubility of iron compounds increases at lower pH values. The method for iron is an adaptation of the TPTZ Method.

Iodine is used for cleaning and disinfection, and can end up in surface waters through evaporation and rainfall. The method for iodine is an adaptation of Standard Methods for the Examination of Water and Wastewater, 18th Edition, DPD Method.

The **HI97101** photometer is a compact and versatile meter suitable for field or bench measurements, featuring a:

- Sophisticated optical system
- Meter validation using certified CAL Check cuvettes
- Tutorial mode guides the user step-by-step
- Auto logging
- Waterproof IP67, floating case
- GLP features



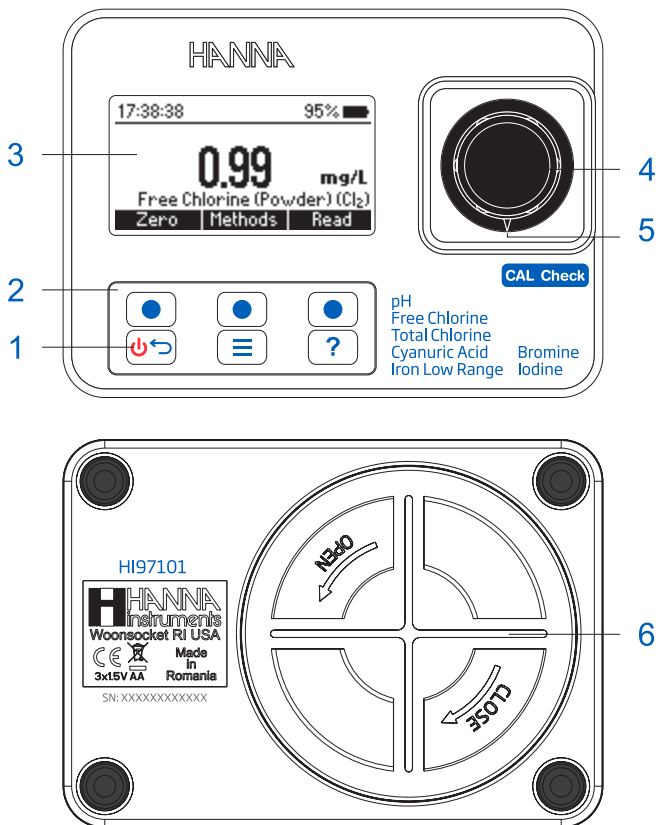

5.2. FUNCTIONAL DESCRIPTION



- | | | |
|------------------------|---------------------------------|------------------|
| 1. ON/OFF power button | 3. Liquid Crystal Display (LCD) | 5. Indexing mark |
| 2. Keypad | 4. Cuvette holder | 6. Battery cover |

Keypad Description

The keypad contains 3 direct keys and 3 functional keys with the following functions:


-  Press the functional key to perform the function displayed above it on the LCD.
-  Press and hold to power off/on. Press briefly to return to the previous screen.
-  Press to access the menu screen.
-  Press to display the context-sensitive help menu.

5.3. PRECISION & ACCURACY

Precision is how closely repeated measurements are to one another. Precision is usually expressed as standard deviation (SD).

Accuracy is defined as the closeness of a test result to the true value and is method specific.

Although good precision suggests good accuracy, precise results can be inaccurate. The figure explains these definitions.

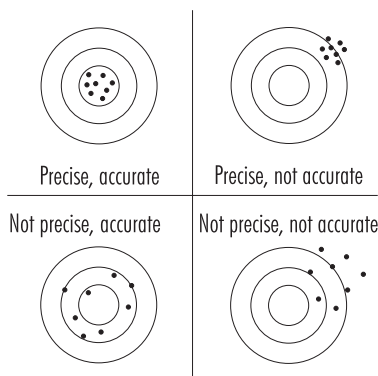

5.4. PRINCIPLE OF OPERATION

Absorption of light is a typical phenomenon of interaction between electromagnetic radiation and matter. When a light beam crosses a substance, some of the radiation may be absorbed by atoms, molecules or crystal lattices. Photometric chemical analysis is based on specific chemical reactions between a sample and reagent to produce a light-absorbing compound.

If pure absorption occurs, the fraction of light absorbed depends both on the optical path length through the matter and on the physical-chemical characteristics of the substance according to the Lambert-Beer Law. If all other factors are constant, the concentration "c" can be calculated from the absorbance of the substance.

Lambert-Beer Law:


$$-\log I/I_0 = \epsilon_{\lambda} c d$$

or

$$A = \epsilon_{\lambda} c d$$

- I_0 = intensity of incident light beam
- I = intensity of light beam after absorption
- ϵ_{λ} = molar extinction coefficient at wavelength λ .
- c = molar concentration of the substance
- d = optical path through the substance

5.5. OPTICAL SYSTEM

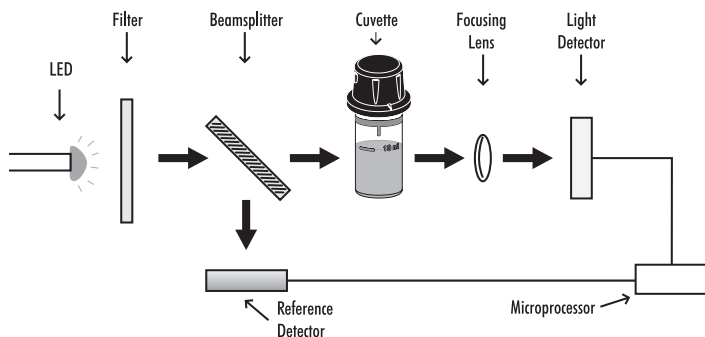

Instrument Block Diagram

The internal reference system (reference detector) of the [HI97101](#) photometer compensates for any drifts due to power fluctuations or ambient temperature changes, providing a stable source of light for your blank (zero) measurement and sample measurement.

LED light sources offer superior performance compared to tungsten lamps. LEDs have a much higher luminous efficiency, providing more light while using less power. They also produce little heat, which could otherwise affect electronic stability. LEDs are available in a wide array of wavelengths, whereas tungsten lamps have poor blue/violet light output.

Improved optical filters ensure greater wavelength accuracy and allow a brighter, stronger signal to be received. The end result is higher measurement stability and less wavelength error.

A focusing lens collects all of the light that exits the cuvette, eliminating errors from cuvette imperfections and scratches, eliminating the need to index the cuvette.

6. GENERAL OPERATIONS

6.1. METER VALIDATION: CAL CHECK & CALIBRATION

Validation of the **HI97101** involves verifying the concentration of the certified CAL Check standards. The CAL Check screen guides the user step-by-step through the validation process and user calibration (if necessary).

WARNING: Do not use any solutions or standards other than the Hanna Instruments® CAL Check Standards. For accurate validation and calibration results, please perform these at room temperature, 18 to 25 °C (64.5 to 77.0 °F).



Note: CAL Check Standards will not read the specified value in measurement mode. Protect the CAL Check cuvettes from direct sunlight by keeping them in the original packing. Store between 5 and 30 °C (41 to 86 °F), do not freeze.

To perform a CAL Check:


1. Press the  key to enter menu. Use the functional keys to select **CAL Check / Calibration** and press **Select**.



The “Not Available” message or the date, time and status of the last CAL Check will be displayed on the screen.



Note: CAL Check & Calibration is for the selected method. Free and Total Chlorine use the same CAL Check & Calibration.

2. Press **Check** to start a new CAL Check. Press the  key at any time to abort the validation process.
3. Use the functional keys to enter the certificate value of the calibration standard found on the CAL Check Standard Certificate. Press **Next** to continue.



Note: This value will be saved in the instrument for future validation. If a new set of calibration standards is obtained, please update the certificate value.

- Insert the **A ZERO** CAL Check Cuvette A then press **Next** to continue. The "Please wait..." message will be displayed during the measurement.









- Insert the CAL Check Cuvette B for the selected method (**HI97710B** for pH, **HI97701B** for Free and Total Chlorine, **HI97722B** for Cyanuric Acid, **HI97746B** for Iron LR, **HI97716B** for Bromine or **HI97718B** for Iodine) then press **Next** to continue. The "Please wait..." message will be displayed during the measurement.











- When the CAL Check is complete, the display will show one of the following messages and the value obtained during the measurement:







- "**PASSED**": The measured value is within the accuracy specification, no user calibration is required.




- “OUT OF SPECIFICATION” and **Calibrate** is available: The measured value is near the expected value. To update the user calibration press **Calibrate**. Press **Accept** to confirm or **Cancel** to return to the previous screen.




- “OUT OF SPECIFICATION”: A user calibration is not allowed, the measured value is outside of the tolerance window. Check the certified value, expiration date and clean the outside of the cuvette. Repeat the CAL Check procedure. If this error continues, contact your nearest Hanna Customer Service Center.



6.2. GLP


Press the  key to enter the menu. Use the functional keys to select **GLP** and press **Select**. Good Laboratory Practice (GLP) shows the date and time of the last user calibration (if available) or factory calibration. To erase the last user calibration and to clear the CAL Check, press **Clear** and follow the prompts. Press **Yes** to erase and return to the factory calibration data or **No** to exit the clear procedure.




6.3. LOGGING DATA & LOG RECALL


The instrument features a data autolog function to help users keep track of all measurements. Every time a measurement is made the data is automatically saved. The data log can hold 50 individual measurements. When the data log is full (50 data points) the meter will rewrite the oldest data point.

Viewing and deleting the data is possible using the **Log Recall** menu.


Press the  key to enter the menu. Use the functional keys to select *Log Recall* and press **Select**.



Use the functional keys to highlight a log and press **Info** to view additional information about the log. From this screen **Next** and **Previous** can be used to view other logs.




Press **Delete** to erase logged data. After pressing **Delete** a prompt on display is asking for confirmation.




Press **No** or the  key to return to the previous screen.

Press **Yes** to delete selected log.


Press **Del All** to erase all the logged data. If **Del All** is pressed, follow the prompt to confirm. Press **Yes** to delete all logged data, **No** or the  key to return to the log recall.



6.4. GENERAL SETUP

Press the  key to enter the menu. Use the functional keys to select *Setup* and press **Select**. Use the functional keys to highlight desired option.

Backlight


Option: 0 to 100 %



Press **Modify** to access the backlight intensity. Use the functional keys to increase or decrease the value. Press **Accept** to confirm or the  key to return to the *Setup* menu without saving the new value.



Contrast

Option: 0 to 100 %



Press **Modify** to change the display's contrast. Use the functional keys to increase or decrease the value. Press **Accept** to confirm the value or the  key to return to the *Setup* menu without saving the new value.



Date & Time

Press **Modify** to change the date and time. Press the functional keys to highlight the value to be modified (year, month, day, hour, minute or second). Press **Edit** to modify the highlighted value. Use the functional keys to change the value.


Press **Accept** to confirm or the  key to return to the previous screen.




Time Format


Option: AM/PM or 24-hour

Press the functional key to select the desired time format.



Date Format


Press **Modify** to change the date format. Use the functional keys to select the desired format. Press **Accept** to confirm or the  key to return to the *Setup* menu without saving the new format.



Decimal Separator

Option: Comma (,) or Period (.)

Press the functional key to select the desired decimal separator. The decimal separator is used on the measurement screen.



Language


Press **Modify** to change the language. Use the functional keys to select the desired language. Press **Accept** to choose one of the languages installed.



Beeper

Option: Enable or Disable


When enabled, a short beep is heard every time a key is pressed. A long beep alert sounds when the pressed key is not active or an error is detected. Press the functional key to enable or disable the beeper.



Tutorial

Option: Enable or Disable


When enabled, the user will be guided step-by-step through the measurement procedure.



Meter Information


Press **Select** to view the model, serial number, firmware version and selected language.

Press the  key to return to the *Setup* menu.





Restore Factory Settings

Press **Select** to reset to factory settings. Press **Accept** to confirm or **Cancel** to exit without restoring the factory settings.





6.5. REAGENTS & ACCESSORIES

Press the  key to enter the menu. Use the functional keys to select *Reagents / Accessories* and press **Select** to access a list of reagents and accessories. To exit press the  key.




6.6. CONTEXTUAL HELP

The HI97101 offers an interactive contextual help mode that assists the user at any time. To access the help screen press the  key.




The instrument will display additional information related to the current screen. To read all the available information, scroll the text using the functional keys.

To exit help mode press the  or the  key and the meter will return to the previous screen.


6.7. BATTERY MANAGEMENT

The meter will perform an auto-diagnostic test when it is powered on. During this test, the Hanna Instruments® logo will appear on the LCD. If the auto-diagnostic test was successful, the meter is ready for use. The battery icon on the LCD will indicate the battery status:


- battery full



- battery below 10%, replace the batteries soon



- battery is low, replace the batteries with new ones




To conserve battery, the meter will turn off automatically after 15 minutes of inactivity. If a zero reading has been done but not a read, auto-off time is increased to 30 minutes.

7. PHOTOMETER

7.1. METHOD SELECTION

Press **Methods** when in measurement mode to access the list of methods. Use the functional keys to highlight the desired method then press **Select**.




The selected method will be saved when the instrument is powered off.

7.2. COLLECTING & MEASURING REAGENTS AND SAMPLES


Proper Use of Powder Packet

1. Use scissors to open the powder packet.
2. Push the edges of the packet to form a spout.
3. Pour out the content of the packet.

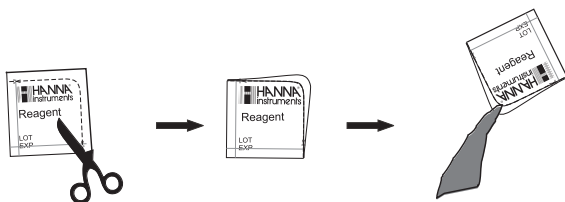

Proper Use of Dropper Bottle


1. Tap the dropper on the table several times and wipe the outside of the tip with a cloth.
2. Always keep the dropper bottle in a vertical position while dosing the reagent.

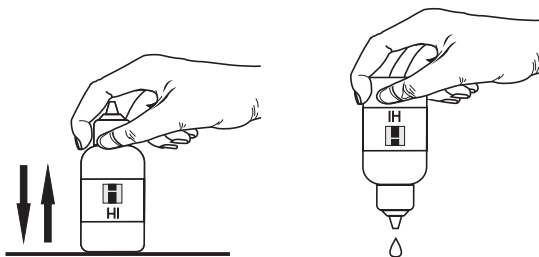

7.3. CUVETTE & CYLINDER PREPARATION

Proper mixing is very important for reproducibility of the measurements. The proper mixing technique for each method is listed in the method procedure.


- (a) The mixing method is indicated with “shake vigorously” using one of the following icons:

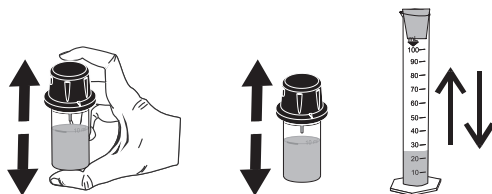


- (b) The mixing method is indicated with “shake gently” using one of the following icons:



- (c) The mixing method is indicated with “swirl” using one of the following icons:

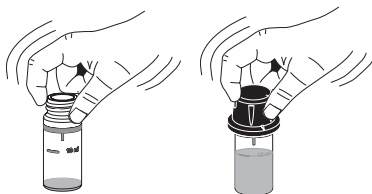

In order to avoid reagent leaking and to obtain more accurate measurements, close the cuvette first with the supplied HDPE plastic stopper  and then the black cap.



Whenever the cuvette is placed into the measurement holder, it must be dry outside and free of fingerprints, oil or dirt. Wipe it thoroughly with HI731318 microfiber cleaning cloth or a lint-free wipe prior to insertion.



Shaking the cuvette can generate bubbles in the sample, causing higher readings. To obtain accurate measurements, remove such bubbles by swirling or by gently tapping the cuvette.

Do not let the reacted sample stand too long after reagent has been added. For best accuracy, respect the timings described in each specific method.

It is possible to take multiple readings in a row, but it is recommended to take a new zero reading for each sample and to use the same cuvette for zeroing and measurement when possible.

Discard the sample immediately after the reading has been taken, or the glass might become permanently stained.

All the reaction times reported in this manual are at 25 °C (77 °F). In general, the reaction time should be increased for temperatures lower than 20 °C (68 °F), and decreased for temperatures higher than 25 °C (77 °F).

8. METHOD PROCEDURE

8.1. pH

REQUIRED REAGENTS

Code	Description	Quantity
HI93710-0	pH Reagent	5 drops

REAGENT SETS

HI93710-01 pH Reagent - 100 tests

HI93710-03 pH Reagent - 300 tests

For other accessories see ACCESSORIES section.

MEASUREMENT PROCEDURE


- Select the pH method using the procedure described in the METHOD SELECTION section.

Note: If tutorial mode is disabled, follow the measurement procedure below. If the tutorial mode is enabled, press **Measure** and follow the messages on the screen.




- Fill the cuvette with 10 mL of unreacted sample (up to the mark). Replace the plastic stopper and the cap.




- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.




- Press **Zero**. The display will show “-0.0-” when the meter is zeroed and ready for measurement.






- Remove the cuvette.
- Add 5 drops of **HI93710-0** pH Reagent indicator. Replace the plastic stopper and the cap. Swirl to mix.



- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.



- Press **Read** to start the reading. The instrument displays the results in pH.



8.2. FREE CHLORINE (POWDER REAGENT)

Note: Free and Total Chlorine have to be measured separately with fresh unreacted samples following the related procedures, if both values are desired.

REQUIRED REAGENTS

Code	Description	Quantity
HI93701-0	Free Chlorine Reagent	1 packet

REAGENT SETS

HI93701-01	Free Chlorine Reagent - 100 tests
HI93701-03	Free Chlorine Reagent - 300 tests

For other accessories see ACCESSORIES section.

MEASUREMENT PROCEDURE


- Select the **Free Chlorine (Powder)** method using the procedure described in the METHOD SELECTION section.

*Note: If tutorial mode is disabled, follow the measurement procedure below. If the tutorial mode is enabled, press **Measure** and follow the messages on the screen.*




- Fill the cuvette with 10 mL of unreacted sample (up to the mark). Replace the plastic stopper and the cap.




- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.




- Press **Zero**. The display will show “-0.0-” when the meter is zeroed and ready for measurement.






- Remove the cuvette.
- Add the content of one packet of **HI93701-0** Free Chlorine Reagent. Replace the plastic stopper and the cap. Shake gently for 20 seconds.

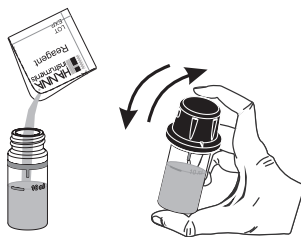

- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.



- Press **Read**. The display will show a 1 minute countdown prior to the measurement. To skip the timer, press **Read** twice. When the timer ends, the meter will perform the reading. The instrument displays the results in **mg/L** of chlorine (Cl_2).



INTERFERENCES

Interference may be caused by:

- Bromine, Iodine, Oxidized forms of Chromium and Manganese, Ozone
- Hardness greater than 500 mg/L CaCO_3 , to remove the interference shake the sample for approximately 2 minutes after adding the powder reagent
- Alkalinity greater than 250 mg/L CaCO_3 or acidity value greater than 150 mg/L CaCO_3 , the color of the sample may develop only partially or rapidly fade, to remove the interference neutralize the sample with diluted HCl or NaOH

8.3. FREE CHLORINE (LIQUID REAGENT)

Note: Free and Total Chlorine have to be measured separately with fresh unreacted samples, following the related procedures, if both values are desired.

REQUIRED REAGENTS

Code	Description	Quantity
HI93701A-F	Free Chlorine Reagent A	3 drops
HI93701B-F	Free Chlorine Reagent B	3 drops

REAGENT SETS

HI93701-F Free Chlorine Reagent - 300 tests

For other accessories see ACCESSORIES section.

MEASUREMENT PROCEDURE


- Select the **Free Chlorine (Liquid)** method using the procedure described in the METHOD SELECTION section.

*Note: If tutorial mode is disabled, follow the measurement procedure below. If the tutorial mode is enabled, press **Measure** and follow the messages on the screen.*




- Fill the cuvette with 10 mL of unreacted sample (up to the mark). Replace the plastic stopper and the cap.




- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.




- Press **Zero**. The display will show “-0.0-” when the meter is zeroed and ready for measurement.




- Remove the cuvette.
- To an empty cuvette add 3 drops of HI93701A-F Free Chlorine Reagent A and 3 drops of HI93701B-F Free Chlorine Reagent B.




- Swirl gently to mix.






- Add 10 mL of unreacted sample (up to the mark). Replace the plastic stopper and the cap. Shake gently to mix.



- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.



- Press **Read**. The display will show a 1 minute countdown prior to the measurement. To skip the timer, press **Read** twice. When the timer ends, the meter will perform the reading. The instrument displays the results in **mg/L of chlorine (Cl₂)**.



INTERFERENCES

Interference may be caused by:

- Bromine, Iodine, Oxidized forms of Chromium and Manganese, Ozone
- Hardness greater than 500 mg/L CaCO_3 , to remove the interference shake the sample for approximately 2 minutes after adding the powder reagent
- Alkalinity greater than 250 mg/L CaCO_3 or acidity value greater than 150 mg/L CaCO_3 , the color of the sample may develop only partially or rapidly fade, to remove the interference neutralize the sample with diluted HCl or NaOH

8.4. TOTAL CHLORINE (POWDER REAGENT)

Note: Free and Total Chlorine have to be measured separately with fresh unreacted samples, following the related procedures, if both values are desired.

REQUIRED REAGENTS

Code	Description	Quantity
HI93711-0	Total Chlorine Reagent	1 packet

REAGENT SETS

HI93711-01 Total Chlorine Reagent - 100 tests

HI93711-03 Total Chlorine Reagent - 300 tests

For other accessories see ACCESSORIES section.

MEASUREMENT PROCEDURE


- Select the **Total Chlorine (Powder)** method using the procedure described in the METHOD SELECTION section.

Note: If tutorial mode is disabled, follow the measurement procedure below. If the tutorial mode is enabled, press **Measure** and follow the messages on the screen.




- Fill the cuvette with 10 mL of unreacted sample (up to the mark). Replace the plastic stopper and the cap.




- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.




- Press **Zero**. The display will show “-0.0-” when the meter is zeroed and ready for measurement.






- Remove the cuvette.
- Add 1 packet of **HI93711-0** Total Chlorine Reagent. Replace the plastic stopper and the cap. Shake gently for 20 seconds.



- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.



- Press **Read**. The display will show a 2 minute 30 second countdown prior to the measurement. To skip the timer, press **Read** twice. When the timer ends, the meter will perform the reading. The instrument displays the results in **mg/L** of chlorine (Cl_2).



INTERFERENCES

Interference may be caused by:

- Bromine, Iodine, Oxidized forms of Chromium and Manganese, Ozone
- Hardness greater than 500 mg/L CaCO_3 , to remove the interference shake the sample for approximately 2 minutes after adding the powder reagent
- Alkalinity greater than 250 mg/L CaCO_3 or acidity greater than 150 mg/L CaCO_3 , the color of the sample may develop only partially or may rapidly fade, to remove the interference neutralize the sample with diluted HCl or NaOH

8.5. TOTAL CHLORINE (LIQUID REAGENT)

Note: Free and Total Chlorine have to be measured separately with fresh unreacted samples, following the related procedures, if both values are desired.

REQUIRED REAGENTS

Code	Description	Quantity
HI93701A-T	Total Chlorine Reagent A	3 drops
HI93701B-T	Total Chlorine Reagent B	3 drops
HI93701C-T	Total Chlorine Reagent C	1 drop

REAGENT SETS

HI93701-T Total Chlorine Reagent - 300 tests

For other accessories see ACCESSORIES section.

MEASUREMENT PROCEDURE


- Select the **Total Chlorine (Liquid)** method using the procedure described in the METHOD SELECTION section.

Note: If tutorial mode is disabled, follow the measurement procedure below. If the tutorial mode is enabled, press **Measure** and follow the messages on the screen.




- Fill the cuvette with 10 mL of unreacted sample (up to the mark). Replace the plastic stopper and the cap.




- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.



- Press **Zero**. The display will show “-0.0-” when the meter is zeroed and ready for measurement.




- Remove the cuvette.
- To an empty cuvette add 3 drops of **HI93701A-T** Total Chlorine Reagent A, 3 drops of **HI93701B-T** Total Chlorine Reagent B, and 1 drop of **HI93701C-T** Total Chlorine Reagent C.

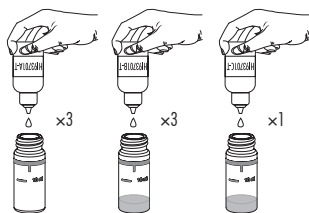


- Swirl gently to mix.






- Add 10 mL of unreacted sample (up to the mark). Replace the plastic stopper and the cap. Shake gently to mix.



- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.



- Press **Read**. The display will show a 2 minute 30 second countdown prior to the measurement. To skip the timer, press **Read** twice. When the timer ends, the meter will perform the reading. The instrument displays the results in **mg/L** of chlorine (Cl_2).



INTERFERENCES

Interference may be caused by:

- Bromine, Iodine, Oxidized forms of Chromium and Manganese, Ozone
- Hardness greater than 500 mg/L CaCO_3 , to remove the interference shake the sample for approximately 2 minutes after adding the powder reagent
- Alkalinity greater than 250 mg/L CaCO_3 or acidity greater than 150 mg/L CaCO_3 , the color of the sample may develop only partially or may rapidly fade, to remove the interference neutralize the sample with diluted HCl or NaOH

8.6. CYANURIC ACID

REQUIRED REAGENTS

Code	Description	Quantity
HI93722-0	Cyanuric Acid Reagent	1 packet

REAGENT SETS

HI93722-01 Cyanuric Acid Reagent - 100 tests

HI93722-03 Cyanuric Acid Reagent - 300 tests

For other accessories see ACCESSORIES section.

MEASUREMENT PROCEDURE


- Select the **Cyanuric Acid** method using the procedure described in the METHOD SELECTION section.

*Note: If tutorial mode is disabled, follow the measurement procedure below. If the tutorial mode is enabled, press **Measure** and follow the messages on the screen.*




- Fill the first cuvette with 10 mL of unreacted sample (up to the mark). Replace the plastic stopper and the cap.




- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.



- Press **Zero**. The display will show “-0.0-” when the meter is zeroed and ready for measurement.



- Fill a beaker with 25 mL sample (up to the mark).




- Add the content of one packet of **HI93722-0** Cyanuric Acid Reagent and mix to dissolve.






- Fill the second cuvette with 10 mL of the reacted sample (up to the mark). Replace the plastic stopper and the cap.



- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.



- Press **Read**. The display will show a 45 second countdown prior to the measurement. To skip the timer, press **Read** twice. When the timer ends, the meter will perform the reading. The instrument displays the results in **mg/L** of cyanuric acid.



8.7. IRON LOW RANGE

REQUIRED REAGENTS

Code	Description	Quantity
HI93746-0	Iron LR Reagent	2 packets

REAGENT SETS

HI93746-01 Iron LR Reagent - 50 tests

HI93746-03 Iron LR Reagent - 150 tests


For other accessories see ACCESSORIES section.

MEASUREMENT PROCEDURE


- Select the **Iron LR** method using the procedure described in the METHOD SELECTION section.

Note: If tutorial mode is disabled, follow the measurement procedure below. If the tutorial mode is enabled, press **Measure** and follow the messages on the screen.

- Fill one graduated mixing cylinder, up to the 25 mL mark, with DIW.




- Add the content of one packet of **HI93746-0** Iron LR Reagent. Close the cylinder with a rubber stopper and shake vigorously for 30 seconds. This is the blank.






- Fill a cuvette with 10 mL of the blank (up to the mark). Replace the plastic stopper and the cap.




- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.




- Press **Zero**. The display will show “-0.0-” when the meter is zeroed and ready for measurement.



- Remove the cuvette.
- Fill another graduated mixing cylinder, up to the 25 mL mark, with the sample.




- Add the content of one packet of **HI93746-0** Iron LR Reagent. Close the cylinder with a rubber stopper and shake vigorously for 30 seconds. This is the reacted sample.






- Fill a cuvette with 10 mL of the reacted sample (up to the mark). Replace the plastic stopper and the cap.



- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.



- Press **Read**. The display will show a 30 second countdown prior to the measurement. To skip the timer, press **Read** twice. When the timer ends, the meter will perform the reading. The instrument displays concentration in **mg/L** of iron (**Fe**).



INTERFERENCES

Interference may be caused by:

- Manganese above 50.0 mg/L
- Cadmium, Molybdenum above 4.0 mg/L
- Cyanide above 2.8 mg/L
- Chromium(VI) above 1.2 mg/L
- Nickel above 1.0 mg/L
- Nitrite ion above 0.8 mg/L
- Copper above 0.6 mg/L
- Mercury above 0.4 mg/L
- Chromium(III) above 0.25 mg/L
- Cobalt above 0.05 mg/L
- Sample pH should be between 3 and 4 to avoid fading or turbidity formation

8.8. BROMINE

REQUIRED REAGENTS

Code	Description	Quantity
HI93716-0	Bromine Reagent	1 packet

REAGENT SETS

HI93716-01 Bromine Reagent - 100 tests

HI93716-03 Bromine Reagent - 300 tests

For other accessories see ACCESSORIES section.

MEASUREMENT PROCEDURE


- Select the **Bromine** method using the procedure described in the METHOD SELECTION section.

Note: If tutorial mode is disabled, follow the measurement procedure below. If the tutorial mode is enabled, press **Measure** and follow the messages on the screen.




- Fill the cuvette with 10 mL of unreacted sample (up to the mark). Replace the plastic stopper and the cap.



- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.




- Press **Zero**. The display will show “-0.0-” when the meter is zeroed and ready for measurement.




- Remove the cuvette.


- Add the content of one packet of **HI93716-0** Bromine Reagent. Replace the plastic stopper and the cap and shake gently for about 20 seconds to dissolve most of the reagent.



- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.



- Press **Read**. The display will show a 2 minute and 30 second countdown prior to the measurement. To skip the timer, press **Read** twice. When the timer ends, the meter will perform the reading. The instrument displays the results in **mg/L of bromine (Br₂)**.



INTERFERENCES

Interference may be caused by:

- Chlorine, Iodine, Ozone, Oxidized forms of Chromium and Manganese
- Hardness greater than 500 mg/L CaCO₃, to remove the interference shake the sample for approximately 1 minute after adding the reagent
- Alkalinity greater than 300 mg/L CaCO₃ or acidity greater than 150 mg/L CaCO₃, the color of the sample may develop only partially or rapidly fade, to remove the interference neutralize the sample with diluted HCl or NaOH

8.9. IODINE

REQUIRED REAGENTS

Code	Description	Quantity
HI93718-0	Iodine Reagent	1 packet

REAGENT SETS

HI93718-01 Iodine Reagent - 100 tests

HI93718-03 Iodine Reagent - 300 tests

For other accessories see ACCESSORIES section.

MEASUREMENT PROCEDURE


- Select the **Iodine** method using the procedure described in the METHOD SELECTION section.

Note: If tutorial mode is disabled, follow the measurement procedure below. If the tutorial mode is enabled, press **Measure** and follow the messages on the screen.




- Fill a cuvette with 10 mL of unreacted sample (up to the mark). Replace the plastic stopper and the cap.




- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.




- Press **Zero**. The display will show “-0.0-” when the meter is zeroed and ready for measurement.





- Add one packet of **HI93718-0** Iodine Reagent. Replace the plastic stopper and the cap. Shake gently for about 20 seconds to dissolve most of the reagent.



- Insert the cuvette into the holder and ensure that the notch on the cap is positioned securely in the groove.



- Press **Read**. The display will show a 2 minute and 30 second countdown prior to the measurement. To skip the timer, press **Read** twice. When the timer ends, the meter will perform the reading. The instrument displays the concentration in **mg/L of iodine (I₂)**.



INTERFERENCES


Interference may be caused by:

- Bromine, Chlorine, Oxidized forms of Chromium and Manganese, Ozone
- Hardness greater than 500 mg/L CaCO₃, to remove the interference shake the sample for approximately 2 minutes after adding the reagent
- Alkalinity greater than 250 mg/L CaCO₃ or acidity greater than 150 mg/L CaCO₃, the color of the sample may develop only partially or rapidly fade, to remove the interference neutralize the sample with diluted HCl or NaOH

9. WARNING & ERROR DESCRIPTIONS

The instrument shows clear warning messages when erroneous conditions appear and when measured values are outside the expected range.


The information below provides an explanation of the errors and warnings, and recommended action to be taken.



There is an excess amount of ambient light reaching the detector. Ensure that the notch on the cap is positioned securely in the groove before performing any measurements. If the issue persists, please contact Hanna Instruments technical support.



The sample and the zero cuvettes are inverted. Swap the cuvettes and repeat the measurement.



There is either too much light or the instrument can not adjust the light level. Please check the preparation of the zero cuvette and that the sample does not contain any debris.



The meter is either overheating or its temperature has dropped too low to operate within published accuracy specifications. The meter must be between 0 and 50 °C (32 and 122 °F) to perform any measurements.



Meter temperature has changed significantly since the zero measurement has been performed. The zero measurement must be performed again.




The measured value is outside the limits of the method. Verify that the sample does not contain any debris. Check the sample preparation and the measurement preparation.




Date and time settings have been lost. Please reset the values. If the issue persists, please contact Hanna Instruments technical support.




English is the only available language. Help function is not available. Restart the meter. If the issue persists, please contact Hanna Instruments technical support.



Battery level is too low for the meter to function properly. Replace the batteries with new ones.




Tutorial mode has been enabled in the Setup menu. Press **Continue** and follow the prompt on the screen. Tutorial mode can be disabled in the Setup menu.




A critical error has occurred. Restart the meter. If the issue persists, please contact Hanna Instruments technical support.

10. BATTERY REPLACEMENT

To replace the instrument's batteries, follow these steps:

- Turn the instrument off by pressing and holding the  key.
- Remove the battery cover by turning it counterclockwise.
- Remove the old batteries, replace them with three new 1.5V AA batteries.
- Replace the battery cover, turn it clockwise to close.

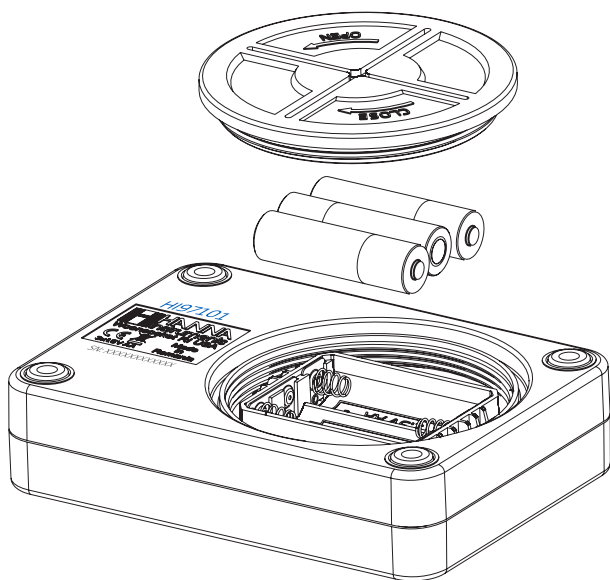

11. ACCESSORIES

11.1. REAGENT SETS

Code	Description
HI93701-01	Free Chlorine Reagent - 100 tests (powder)
HI93701-03	Free Chlorine Reagent - 300 tests (powder)
HI93701-F	Free Chlorine Reagent - 300 tests (liquid)
HI93701-T	Total Chlorine Reagent - 300 tests (liquid)
HI93710-01	pH Reagent - 100 tests
HI93710-03	pH Reagent - 300 tests
HI93711-01	Total Chlorine Reagent - 100 tests (powder)
HI93711-03	Total Chlorine Reagent - 300 tests (powder)
HI93716-01	Bromine Reagent - 100 tests
HI93716-03	Bromine Reagent - 300 tests
HI93718-01	Iodine Reagent - 100 tests
HI93718-03	Iodine Reagent - 300 tests
HI93722-01	Cyanuric Acid Reagent - 100 tests
HI93722-03	Cyanuric Acid Reagent - 300 tests
HI93746-01	Iron LR Reagent - 50 tests
HI93746-03	Iron LR Reagent - 150 tests

11.2. OTHER ACCESSORIES

Code	Description
HI7101417	blue carrying case for HI977xx and 7 CAL Check cuvettes
HI731318	cloth for wiping cuvettes (4 pcs.)
HI731331	glass cuvette (4 pcs.)
HI731336N	cap for cuvette (4 pcs.)
HI740034P	cap for 100 mL beaker (10 pcs.)
HI740036P	plastic beaker (10 pcs.)
HI740220	25 mL graduated glass vial (2 pcs.)
HI740229	100 mL graduated cylinder
HI93703-50	cuvette cleaning solution (230 mL)
HI97701-11	CAL Check [®] standards for Free and Total Chlorine - cuvette kit
HI97710-11	CAL Check [®] standards for pH - cuvette kit
HI97716-11	CAL Check [®] standards for Bromine - cuvette kit
HI97718-11	CAL Check [®] standards for Iodine - cuvette kit
HI97722-11	CAL Check [®] standards for Cyanuric Acid - cuvette kit
HI97746-11	CAL Check [®] standards for Iron LR - cuvette kit

CERTIFICATION

All Hanna Instruments conform to the **CE European Directives**.



Disposal of Electrical & Electronic Equipment. The product should not be treated as household waste. Instead hand it over to the appropriate collection point for the recycling of electrical and electronic equipment which will conserve natural resources.

Disposal of waste batteries. This product contains batteries, do not dispose of them with other household waste. Hand them over to the appropriate collection point for recycling. Ensuring proper product and battery disposal prevents potential negative consequences for the environment and human health. For more information, contact your city, your local household waste disposal service, the place of purchase or go to www.hannainst.com.



RECOMMENDATIONS FOR USERS

Before using this product, make sure it is entirely suitable for your specific application and for the environment in which it is used. Any variation introduced by the user to the supplied equipment may degrade the meter's performance. For yours and the meter's safety do not use or store the meter in hazardous environments.

WARRANTY

The **HI97101** is warranted for two years against defects in workmanship and materials when used for its intended purpose and maintained according to instructions. This warranty is limited to repair or replacement free of charge. Damage due to accidents, misuse, tampering or lack of prescribed maintenance is not covered.

If service is required, contact your local Hanna Instruments Office. If under warranty, report the model number, date of purchase, serial number (engraved on the bottom of the meter) and the nature of the problem. If the repair is not covered by the warranty, you will be notified of the charges incurred. If the meter is to be returned to Hanna Instruments, first obtain a Returned Goods Authorization (RGA) number from the Technical Service department and then send it with shipping costs prepaid. When shipping any meter, make sure it is properly packed for complete protection.

Hanna Instruments reserves the right to modify the design, construction or appearance of its products without advance notice.

World Headquarters

Hanna Instruments Inc.
Highland Industrial Park
584 Park East Drive
Woonsocket, RI 02895 USA
www.hannainst.com



MAN97101

Printed in ROMANIA